



## Adaptation in metal-ceramic and all-ceramic restorations

Adaptation

Davood Mohammadi<sup>1</sup>, Mohsen Movahedzadeh<sup>2</sup>, Saeedi Zahra<sup>3</sup>, Seyedeh Azam Hoseini<sup>4</sup>, Mohammad Bagheri Iraj<sup>2</sup>

<sup>1</sup>Postgraduate student, Department of Pediatrics, School of Dentistry, Shahed University of Medical Sciences, Tehran,

<sup>2</sup>Department of Prosthodontics, School of Dentistry, Mashhad University of Medical Sciences, Mashhad,

<sup>3</sup>Undergraduate student, School of Dentistry, Mashhad University of Medical Sciences, Mashhad,

<sup>4</sup>Department of Restorative Dentistry, School of Dentistry, Mashhad University of Medical Sciences, Mashhad, Iran

### Abstract

**Aim:** Lack of good marginal adaptation in dental restorations over time tends to dissolve the cement in oral cavity, which leads to the accumulation of plaque, tooth decay, pulp contention, gingivitis and periodontal diseases and ultimately treatment failure. The aim of this study is to evaluate and compare the internal and marginal adaptation in metal-ceramic and all-ceramic restorations made by traditional and CAD/CAM methods. **Material and Method:** 1. Preparation of working cast and die 2. Preparation of restorations: In this study the samples were divided into 6 groups of 10, which are as follow: Group A: metal-ceramic restorations without collar made by manual method (traditional and conventional). Group B: metal-ceramic restorations without metal collar, in which the wax coping was made of special blanks by CAD/CAM method and the rest of process is manual. Group C: metal-ceramic restorations without metal collar, in which their frame was made by using dry milling method and Sintron technology and the rest of process was done manually. Group D: E.max-Press all-ceramic restorations (lithium disilicate). Group E: All-ceramic restoration with Core Zirconia prepared by CAD/CAM method and porcelain layering. Group F: Trans-Lucent zirconia (solid) all-ceramic restorations as full-contour by CAM/COD method. 3. Measuring the amount of the gap: Replica technique was used for this purpose. **Results:** The lowest mean gap in marginal and internal restorations was in group B and the highest amount was in Group C and D, respectively, and altogether there was a significant difference between 6 study groups ( $P < 0.001$ ). The mean marginal gap in all groups (except group B) was more than 120 microns, which is not clinically acceptable. The best marginal and internal adaptation was observed in Group A and B. **Discussion:** Based on the findings of this study, traditional spruing technique, investment, wax removing and alloy injection still provide the best marginal adaptation and in general comparison, metal-ceramic restorations are preferred over all-ceramic restorations.

### Keywords

Marginal; Internal; Restoration; Metal-Ceramic; All-Ceramic

DOI: 10.4328/JCAM.5504

Received: 14.04.2017 Accepted: 02.06.2017 Printed: 01.12.2017 J Clin Anal Med 2017;8(suppl 4): 448-53

Corresponding Author: Mohsen Movahedzadeh, Department of Prosthodontics, School of Dentistry, Vakil Abad Blvd, P.O.Box 91735-984, Mashhad, Iran.

E-Mail: Mohsenmovahedzadeh@gmail.com

## Introduction

The milling of abutment teeth is one of the main steps of crown fabrication. milled parts should be covered completely and accurately to prevent onset or recurrence of tooth decay. This is only possible by good adaptation of crown edges with finishing line of teeth milling. Lack of good marginal adaptation in crowns over the time tends to dissolve the cement in oral cavity and provide a way for penetration of micro-organisms and toxins caused from their activities, it also leads to plaque accumulation, recurrent caries, pulp contention, and onset of inflammation in periodontal tissue around the finishing line of teeth milling and ultimately restoration failure. [9, 10, 11]

Restorations are divided into two categories: **1-** metal-ceramic and **2-** all-ceramic. Metal-ceramics melt at relatively low temperature (800 C). Today, with the changes that have been done on metal frame, there has been an attempt to restore the beauty and natural property of metal-ceramics by using investment techniques and very thin coping (2.0 to 3.0 mm) [7]. In a classification system by America Dental Association (ADA) metals used in metal-ceramics are divided into 3 categories: **1-** High noble metals, having more than 60% noble metal (like gold–palladium). **2-**

Noble alloys (35% to 45%) with a small amount of gallium. **3-** Alloys that generally have less than 25% noble metal. Selecting a suitable alloy depends on the factors such as price and stiffness, pouring capability, easy finishing and polishing, resistance to corrosion and compatibility with porcelain. Suitable compounds include gold (44% to 55%) and palladium (35 to 45%) with a small amount of gallium [7]. Metal-ceramic restorations still are the gold standard in fixed denture [16, 17].

All-ceramic restorations (without metal) are increasingly being prescribed to patients, which due to the high aesthetic functionality and histocompatibility features they are great. In order to improve the usability as dental material and to improve the strength and stiffness properties, from 1980 up to now, various ceramic materials and manufacturing techniques were introduced, which lithium disilicate, alumina and zirconia can be named [9, 10, 11]. The method used to build an all-ceramic crown is actually simple, but to create a beautiful, harmonious and functional structure, great skill is required. Of all the all-ceramic systems, Inceram in the best way has all of these factors. This material has the best mechanical properties (almost three times more flexural strength compared to other systems, except Porcera system), Spinell core, which is composed of MgAl<sub>2</sub>O<sub>3</sub>, has natural teeth translucency. Inceram margins fit well (marginal gap depth of 10–40 μm), core transparency is able to cover the undesirable reflection in oral cavity. The problem of using these system is that they require special equipment [6].

Possible errors during the construction of the restorations by CAD/CAM, including process of scanning, designing by software, milling by machine and contraction during sintering, affect the amount of marginal integrity [12–15]. New technology of using designing technology and computer-aided manufacturing (CAD/CAM) for making crowns, laminates and 3-unit anterior fixed partial dentures require precise teeth preparation and molding, in order to be used as a prosthetic repair with margins. This technology often allows us to complete various cases, even single tooth restoration, in collaboration with numerous specialist, without the need for direct contact with patient and though electronic communication and memory structures. 4.0

and 6.0 mm coping with different crowning ability and two different materials (zirconia and alumina) and multiple liners can be outlined as features of all-ceramic CAD/CAM crown [8].

The marginal adaptation is one of the essential factors to achieve long-term success for each restoration. As there is not always a precise definition for marginal adaptation, it can be said that the best way to check it is by measuring non-adaptation of different areas of prepared teeth to edge of the crown [1–5]. Lack of marginal adaptation can be due to inaccuracies in the fabrication of crown, lack of full sitting during cementation of it or a combination of both. The aim of this study is to evaluate and compare the marginal and internal adaptation in metal-ceramic and manual all-ceramic (conventional) and CAD/CAM restorations.

In a study by A.M. Fahmy et al. (2012) on marginal adaptation of metal-ceramic restorations without metal collar and IPS Empress CAD/CAM restorations, it was revealed that metal-ceramic restorations without metal collar have the best adaptation and they are recommended in important areas in terms of beauty without worrying about the marginal gap [18]. Tamac et al. (2014) in a comparative study for comparing marginal fit of metal-ceramic restorations made with three methods of CAD/CAM, Laser Sinter and conventional casting suggested that each of 3 methods have a similar marginal fit, which are in the range of clinical standard [19]. According to a study by Zhuoli Huang et al. (2015), metal-ceramic crowns made with CAD/CAM technique, Laser-Sinter (chrome – cobalt) and gold–platinum casting had similar margin fitting and chrome–cobalt casting crowns had the least marginal adaptation [20]. Nejatidanesht et al. (2016) examined the marginal and internal adaptation of implant-supported restoration made with 2 different methods of CAD/CAM and 2 different traditional methods and from this study concluded that CAD/CAM technology provides better marginal fit.

## Material and Method

In this experimental study to prepare the cast and die, first two maxillary dental arches were selected and first molar tooth above it was prepared for similarity with clinical conditions with a shoulder milling with a depth of approximately 1 mm for full crowning and the tooth was examined with surveyor to ensure that there is no undercut. Then template was prepared from the maxillary and mandibular arches by two perforated metal trays and additive silicone impression material (BONASIL,DMP,Greece) and working cast was obtained by stone gypsum (dentona,dentona AG,Germany) and under vacuum, in which the die was prepared after trimming and sawing (cutting) steps. The above steps were repeated for the preparation of each restoration. 6 groups of 10 and a total of 60 restorations (crowns) were created, in which the restorations of groups A, B and C were metal-ceramics and the restorations of D, E and F were all-ceramics. It should be noted that Group A is the conventionally, manually and controlled group in the study. In order to provide restoration of Group A, after preparing the die, the two layers of Die spacer (mega-Stumpflack,megadental GmbH,Germany) were placed on it, thickness of each layer is 15 microns and is extended up to 1 mm of margin. Cement space for all the samples whether manual or CAD/CAM was considered as 30 microns. Then the wax-up coping was done and the labial margin wax was removed. After completing the

waxing-up, spruing and investing, cylinder was filled with Investment gypsum (CODENT/PODENT,Dandiran,Iran) and cylinders were placed inside the removing wax furnace (SUNNYTHERM-1,KFP,Iran). Then the inductive centrifuge machine (DUCATRON,KFP,Iran) was used for melting and casting of molten chrome-cobalt alloy (NEW CAST,YAMAHACHI DENTAL MFG,Japan) into the productive space and then it was allowed to become cool. Clean investment gypsum and sandblasting were used for the final cleanup. Feldspathic porcelain layering (Super porcelain EX-3,NORITAKE CO,Japan) was done according to its routine. Placing of opaque layer, shoulder porcelain (initial,GC,E.U) with Direct Lift technique (direct removal of restorations from top of die and direct placement of shoulder porcelain), dentin and enamel and finally firing the porcelain in the special furnace (Programat P500,IVOCLAR VIVADENT, Liechtenstein) were completed and then contacts and occlusions were set according to the opposite arc and adjacent teeth. Wax copings from special wax blanks for milling with COD/CAM (Ceramill wax,Amann) were used to prepare the restorations of the Group B. Casts were scanned with Scanner (Ceramill map400, Amann GIRRbach , Austria) and processes of CAD/CAM designing were done in computer software. After preparation of wax copings of CAD/CAM milling (imes-icore GmbH,Germany imes-icore 550 i,) the rest of process was similar to group A. Sintron technology was used to prepare the restorations of group C. First the casts were scanned by a scanner. Coping were milled by CAD/CAM machine from soft blanks and gypsum such as chrome-cobalt alloy (Ceramill Sintron,Amann GIRRbach , Austria) and then were placed inside of sinter furnace to sinter and they were put under argon gas pressure (Ceramill Argotherm, Amann GIRRbach , Austria) and they have strength comparable to manual and conventional types. It should be noted that the CAD/CAM milling used in study groups was from soft milling zirconia types (dry milling). To prepare the restorations of group D which are E.max-Press (lithium disilicate or glass-ceramic), a full wax-up was done on samples of this group and then they were placed in wax removal furnace to achieve the productive space. Then Ingots for E.max (IPS e.max, ,IVOCLAR VIVADENT, Liechtenstein) in furnace for Press (Programat EP 3000, ,IVOCLAR VIVADENT, Liechtenstein) were casted into the productive space by special plunger, after cleaning the plaster Investments, an all-ceramic full-contour restoration was obtained. The restorations of group E are Zircon. To prepare the samples of this group, first scanning of casts and processes of CAD/CAM designing were carried out. Then a core zirconia was milled by CAD/CAM from blanks for zirconia (Ceramill Zi,Amann GIRRbach, Austria). Binder was put on it and then special porcelain layering was carried out and porcelain shoulder specific for zirconia was placed in the area of buccal margin and zirconia was put inside of sintering furnace. To prepare the restoration samples of group F, first scanning of casts and processes of CAD/CAM designing were carried out. Name of the restorations of this group is Zolid, which is a translucent zirconia and it was obtained as full-contour from Zolid soft blanks (Ceramill Zolid,Amann GIRRbach,Austria) by CAD/CAM milling and then was put in the furnace for sintering the zirconia. The replica technique was used for measuring the internal and marginal gap. This means that the restoration was filled with additive silicon with light body consolidation (BONASIL,DMP,Greece) and was put on the respective die. Immediately and with caution additions of im-

pression material was cleaned and the restoration was held for 2 minutes with finger pressure (for similarity with clinical conditions). After setting of the impression materials, restoration was removed from the respective die. Thin layer of light body silicon is attached to the inner surface of the restoration, which is actually indicative of the gap in different parts of restoration and in order to strength it and make it examinable, we fill the inside of restoration with Injectable additive silicone with medium or heavy consolidation (BONASIL,DMP,Greece) and let it be set. Then we remove the silicone from inside of restoration and saw whether the light body silicone layer is attached to amplifier silicone, now according to figure this silicone block is milled with a milling razor. 8 cuts are used to examine the points and middle area does not use. Marginal gap is measured at 8 points and internal gap measured at 4 points (cervical, middle of axial level, axial occluso line angle and center of occlusal surface). Light body silicone layer thickness, which is actually equal to amount of the existing gap, is photographed by stereomicroscope (Dino-Lite,Taiwan) with a magnification of 60 times and then it was calculated and declared using Dino Capture 2.0 software. Tables and appropriate statistical charts were used for describing the data and one-factor variance analysis test or its non-parametric equivalent was used for data analysis. The sample size for two independent groups was determined based on the study by Kim Ki-Baek et al. (2014) with 85% power and 10 samples in each group [22].

## Results

In this study, three variables of internal, marginal and buccal marginal adaptations were examined between six groups as well as between metal-ceramic and all-ceramic restorations. The normality of the data was evaluated using the Shapiro-Wilk test and it was determined that the data for some variables and some groups are not normally distributed. The results showed that for the internal adaptation, range of data changes of group 4 is much greater than the other groups. The lowest value observed belongs to group 6 and the highest values belongs to group 4. The lowest mean belongs to group 2 and the highest mean belongs to group 4, the lowest mean value belongs to group 1 and the highest mean value belongs to group 3. In total, the distributions among 6 groups are significantly different with each other ( $P < 0.001$ ), which in pairwise comparison of groups with each other, it was determined that groups 1, 2 and 3 were significantly lower than groups 3 and 4. Group 6 was significantly lower than group 4, group 3 was also significantly lower than group 4. There was no significant difference between the other groups (Table 1).

Table 1. The mean, standard deviation, minimum, maximum and median of data for internal adaptation in study groups and statistical test result

Group	Numbers	Mean	Standard deviation	Lowest	Highest	Median	Kruskal-Wallis test result
1	320	113.77	52.44	30.61	329.63	98.21	
2	320	112.40	53.44	43.44	336.71	99.23	
3	320	149.85	99.66	43.44	792.80	159.18	$\chi^2=153.04$ $P<0.001$
4	320	172.25	115.76	54.30	1650.76	139.26	
5	320	117.80	46.84	46.07	314.92	127.29	
6	320	120.72	53.39	26.02	292.40	131.21	

Based on the results of marginal adaptation data, range of data changes in group 3 is greater than other groups. The lowest value observed belongs to group 2 and the highest belongs to group 3. The lowest mean belongs to group 2 and the highest belongs to group 3, the lowest median belongs to group 2 and the highest belongs to group 5. In total, the distributions among 6 groups are significantly different with each other ( $P < 0.001$ ), which in pairwise comparison of groups with each other, it was determined that group 2 is significantly lower than other groups. Group 1 was significantly lower than group 3, 5 and 6. There was no significant difference between the other groups (Table 2).

Table 2. The mean, standard deviation, minimum, maximum and median of data for marginal adaptation of the study groups and the statistical test result

Group	Num- bers	Mean	Standard devia- tion	Lowest	Highest	Median	Kruskal- Wallis test result
1	80	135.42	69.34	49.79	372.33	106.91	X <sup>2</sup> =122.36 P<0.001
2	80	92.49	54.80	39.15	369.38	72.85	
3	80	195.17	123.33	54.30	680.33	152.41	
4	80	155.92	73.70	69.53	607.05	136.71	
5	80	181.05	85.55	65.16	602.08	179.86	
6	80	168.72	54.11	87.56	347.67	165.04	

The box chart below shows the distribution of data for internal and marginal adaptation with separation of study groups. As it can be seen, there is a large distribution in groups of 1, 3 and 4, and there are large outlier values in the data for marginal adaptation of groups 3 and 5 (chart 1).

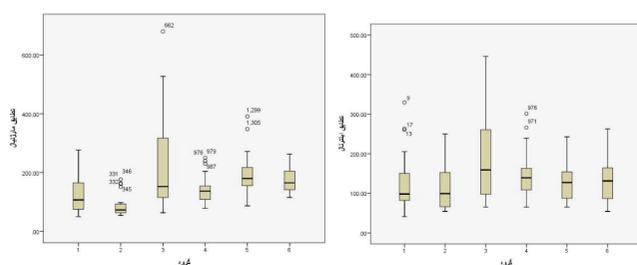


Chart 1. The distribution of Internal and marginal adaptation, with separation of study groups

The range of data changes in buccal marginal adaptation data for groups 5 is higher than other groups. The lowest value belongs to group 2 and the highest belongs to group 5. The lowest mean belongs to group 2 and the highest belongs to group 5, the lowest median value belongs to group 2 and the highest belongs to group 3. In total, the distribution among 6 groups are significantly different with each other ( $P < 0.001$ ), which in pairwise comparison of groups with each other, it was determined that group 2 is significantly lower than other groups. There was no significant difference between the other groups (Table 3). The box chart below shows the distribution of data for buccal marginal adaptation with separation of study groups. As it can be seen, there are large outlier values (chart 2).

Table 3. The mean, standard deviation, minimum, maximum and median in the study groups and the statistical test result

Group	Num- bers	Mean	Standard deviation	Lowest	Highest	Median	Kruskal- Wallis test result
1	30	155.21	81.45	61.21	372.33	121.48	X <sup>2</sup> =33.37 P<0.001
2	30	96.22	58.97	39.15	342.18	82.31	
3	30	174.43	87.98	54.30	414.65	169.11	
4	30	144.42	51.42	69.53	262.65	148.48	
5	30	183.21	118.36	65.16	602.08	152.99	
6	30	158.62	34.37	87.56	222.81	159.03	

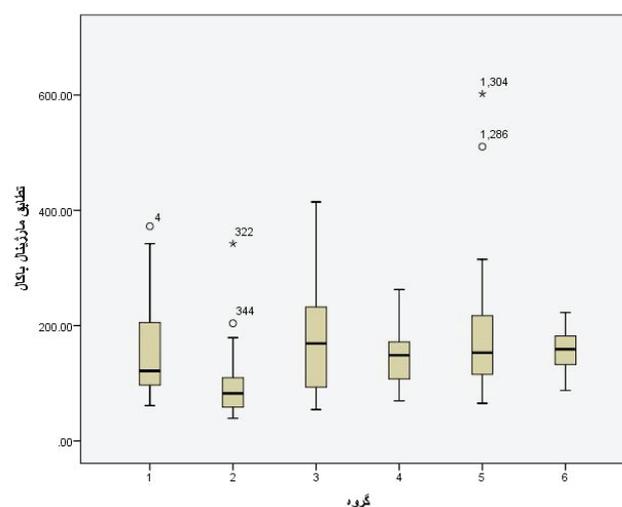


Chart 2. The distribution of data for buccal marginal adaptation with separation of study groups.

The results of the marginal adaptation data indicated that range of data changes in all-ceramic group is lower than metal-ceramic group. The lowest and the highest value observed belongs to metal-ceramic group. The lower mean and median belongs to metal-ceramic group and the higher mean belongs to all-ceramic group. The difference between the two groups was statistically significant ( $P < 0.001$ ) (Table 4).

Table 4. The mean, standard deviation, highest, lowest and median of marginal adaptation data in metal-ceramic and all-ceramic groups and statistical test result.

Group	Num- bers	Mean	Stan- dard devia- tion	Low- est	Highest	Median	Mann- Whitney test result
Metal- ceramic	240	141.03	96.90	39.15	680.33	105.92	Z=6.93 P<0.001
All-ce- ramic	240	168.57	70.66	65.16	607.05	155.49	

As shown in Table 5, range of data changes in all-ceramic group is higher than metal-ceramic group. The lowest and highest value observed belongs to all-ceramic group. The lower mean and median belongs to metal-ceramic group and higher mean belongs to all-ceramic group. The difference between the two groups is statistically significant ( $P < 0.001$ ).

Table 5. The mean, standard deviation, highest, lowest and median of internal adaptation data in metal-ceramic and all-ceramic groups and statistical test result.

Group	Numbers	Mean	Standard deviation	Lowest	Highest	Median	Mann-Whitney test result
Metal-ceramic	960	125.34	73.96	30.61	792.80	106.93	Z=5.28 P<0.001
All-ceramic	960	136.92	82.23	26.02	1650.76	121.41	

The box chart below shows the distribution of data for internal and marginal adaptation with separation of all-ceramic and metal-ceramic groups (chart 3).

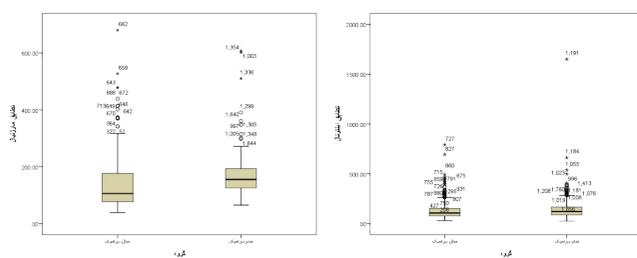


Chart 3. The distribution of data for internal and marginal adaptation with separation of all-ceramic and metal-ceramic groups

## Discussion and Conclusion

Marginal adaptation is one of the key criteria in successful clinical restorations [4-1]. After clinical examination of over a thousand metal-ceramic crowns, Mclean & Von Fraunhofer reported that marginal gap of up to a maximum of 120  $\mu\text{m}$  is acceptable. Other clinicians stated the maximum value as 100  $\mu\text{m}$  [8]. All-ceramic restorations (without metal) are increasingly being prescribed to patients, which is due to their high aesthetic capability and their excellent histocompatibility properties [9, 10, 11]. Possible errors during the construction of the restorations with CAD/CAM, including process scanning, designing by software, milling by machine and contraction during sintering, affect the amount of marginal adaptation [12 – 15].

The aim of this study was to evaluate and compare the marginal adaptation in metal-ceramic and all-ceramic CAD/CAM restorations. Therefore, in this study, a total of 60 dies created from milled molar teeth were prepared on the arch and dies were divided to 6 groups of 10, in which metal-ceramic restorations for 3 groups and all-ceramic restorations were made in the following order: in group A, all-ceramic restorations were made in the traditional way and this group considered as control group. In group B, wax copings were made from millable wax blocks by CAD/CAM machine and after making of metal coping, porcelain was done by conventional method. In group C, Sintron technology was used, in which metal copings are prepared from chrome-cobalt alloys milled by CAM/CAD machine. In group D, E.max press restorations were used. Zircon restorations were made for group E and Zolid restorations were made for group F and for all of the samples of study, the internal, marginal and buccal marginal adaptations were measured using gap measuring by Replica technique. The results showed that the best internal, marginal and buccal marginal were observed in groups 1 and 2. This finding suggests that using traditional techniques of spruing, investment, wax elimination and alloy casting provide the

best marginal adaptation. Vojdani et al. (2013) examined the internal and marginal adaptations in metal-ceramic restorations which are made by traditional method by using CAD/CAM. They prepared 12 copings by CAD/CAM method and 12 copings by traditional method and measured the internal and marginal adaptations in 15 points. In this study, they concluded that the internal and marginal adaptation in metal-ceramic made by traditional method is significantly better than the internal and marginal adaptation in metal-ceramic made by CAD/CAM [23]. The mean internal, marginal and buccal marginal adaptations for teeth in group C were 148.9, 195.17 and 174.4, respectively, which in overall these amounts are indicative of lesser adaptation of restorations made by Sintron technology compare to other restorations. Also, the lowest internal adaptation was related to group D with the mean of 172.2, which shows that glass-ceramic restorations that are made by lithium disilicate casting into mold space have lesser internal adaptation compare to all-ceramic restorations made by CAD/CAM method. But marginal adaptations in E.max restorations were lesser than restorations made by CAD/CAM. From these findings, we cannot make judgment about advantage of all-ceramic restorations made by CAD/CAM method over E.max restorations. Among the metal-ceramic restorations, restorations made by Sintron technology had the worst adaptation. But in comparison with restorations of A and B, internal adaptation in these two groups were the same, but marginal gap in group B, in which wax blocks were made by CAD/CAM technology, was significantly lesser than restorations made by traditional method. These finding could be indicative of priority of metal-copings that their wax pattern is made by CAD/CAM method. Since there is a general agreement among researchers about clinically acceptable gap of less than 120  $\mu\text{m}$  [8, 29], based on the findings of our study, only the adaptations in group B are acceptable. Several studies have examined the different methods of preparing all-ceramic restorations made by CAD/CAM method in terms of marginal adaptation. According to the findings of the study by Paolo Vigolo, Seven Reich and Beuer, different methods of preparing all-ceramic restorations by CAD/CAM have no significant difference in terms of marginal adaptation and in all of these study, marginal gap was clinically acceptable at the end [24, 25, 26]. In the study by kohorstp et al. (2009), in which they examine the marginal precision of 4-unit zirconia restorations made by different CAM/CAD methods (Digident, Inlab, Everest, Cercon) before and after sintering, it was determined that the marginal adaptation of zirconia is highly dependent on used CAM/CAD system and restorations prior to sintering have better marginal adaptation [27]. Kianoosh Torabi et al. (2011) examined the zirconia copings made by CAD/CAM and Slip-Cast in terms of marginal adaptation and suggested that CAD/CAM is competitive with conventional methods and clinically and in vitro has acceptable marginal adaptation [28]. In comparison of marginal adaptation of 3-unit restorations with two methods of Laser sintering and Lost Wax which was conducted by Ki-Baek Kim (2013), It was determined that the marginal adaptation of conventional method (Lost Wax) is significantly better and marginal adaptation of Laser sintering method is not clinically acceptable [29]. On the study by Zhuoli Huang et al. (2014), it was determined that Laser-sinter metal-ceramic restorations have better marginal adaptation compare to CAM/CAD method (both zirconia and disilicate system) [20].

In this study, results showed that there is no difference between two methods of preparing all-ceramic restorations by CAD/CAM machine. But in all 3 groups of all-ceramic restorations, the mean of internal and marginal gap was more than 120  $\mu\text{m}$ , which according to many researchers is not clinically acceptable. Perhaps we could associate the difference between this finding of our study and some studies [14, 30, 31, 32] with difference in preparing restorations, as in these studies measuring the gap on restorations were performed prior to sintering, while in our study, all-ceramic restorations after preparation undergone sintering again. According to the findings of study by Vigolo, restorations prepared by CAD/CAM technique, prior to sintering have better adaptation compare to restorations post sintering. General comparison of metal-ceramic and all-ceramic restorations was also indicative of priority of internal and marginal adaptation of metal-ceramic restorations over all-ceramic restorations. The findings of this study, regarding better internal and marginal adaptation of metal-ceramic restorations compare to all-ceramic restorations, were similar to other studies [26, 27, 33, 34].

Comparing the results of different studies conducted on marginal adaptation of restorations is difficult, because these studies have significant differences, for example, some studies have been conducted in vitro, some on clinical samples, some on single-unit restorations and some other on multi-unit restorations. There are considerable differences in the details of laboratory procedures and materials used in these studies, in addition, different methods of measuring the marginal gap of restoration, itself can be a source of difference between results of different studies.

### Competing interests

The authors declare that they have no competing interests.

### References

1. Beuer F, Schweiger J, Edelhoff D. Digital dentistry: an overview of recent developments for CAD/CAM generated restorations. *Br Dent J* 2008;204:505–11.
2. Raigrodski AJ, Chiche GJ. All-ceramic fixed partial dentures. Part I: in vitro studies. *J Esthet Restor Dent* 2002;14:188–91.
3. Cenci MS, Pereira-Cenci T, Donassollo TA, Sommer L, Strapasson A, Demarco FF. Influence of thermal stress on marginal integrity of restorative materials. *Journal of Applied Oral Science*. 2008;16(2):106–10.
4. Kohorst P, Herzog TJ, Borchers L, Stiesch-Scholz M. Loadbearing capacity of all-ceramic posterior four-unit fixed partial dentures with different zirconia frameworks. *Eur J Oral Sci*. 2007;115:161–6.
5. Tinschert J, Natt G, Mautsch W, Augthun M, Spiekermann H. Fracture resistance of lithium disilicate-, alumina-, and zirconia-based three-unit fixed partial dentures: a laboratory study. *Int J Prosthodont* 2001;14:231–38.
6. Luthy H, Filser F, Loeffel O, Schumacher M, Gauckler L, Hammerle CH. Strength and reliability of four unit all-ceramic posterior bridges. *Dent Mater* 2005;21:930–7.
7. Sailer I, Feher A, Filser F, Gauckler LJ, Luthy H, Hammerle CH. Five-year clinical results of zirconia frameworks for posterior fixed partial dentures. *Int J Prosthodont* 2007; 20:383–8.
8. McLean JW. The science and art of dental ceramics. Vol 1: The nature of dental ceramics and their clinical use. Chicago, IL: Quintessence International; 1979, pp. 63–71.
9. Troia MG, Henriques GEP, Nobilo MAA, Mesquita MF. The effect of thermal cycling on the bond strength of low-fusing porcelain to commercially pure titanium-aluminum-vanadium alloy. *Dental Materials* 2003; 19: 790–6.
10. Stwarczyk B, et al. A Novel CAD/CAM Base Metal Compared to conventional CoCrMo Alloys. *J of Oral Health and Dental Management* 2014;13:2.
11. Rosen Stiel S, Land M, Fujimoto J. Contemporary fixed prosthodontics. 1<sup>st</sup> ed. Louis: Mosby;2001.P.643.
12. Wolf H, Rotei Chack K. color atlas of dental medicine, esthetic dentistry. 1<sup>st</sup> ed. New York: Thieme Stuttgart; 2000.P.163–47.
13. Touati B, Etienne J.M. CAD/CAM all ceramic crowns. *QDT* 2002;25:85–98.
14. El Zohairy AA, De Gee AJ, Mohsen MM, Feilzer AJ. Microtensile bond strength testing of luting cements to prefabricated CAD/CAM ceramic and composite blocks. *Dental Materials*. 2003;19(7):575–83.
15. Willer J, Rossbach A, Weber H-P. Computer-assisted milling of dental restorations using a new CAD/CAM data acquisition system. *The Journal of prosthetic dentistry*. 1998;80(3):346–53.
16. Pettenò D, Schierano G, Bassi F, Bresciano ME, Carossa S. Comparison of marginal fit of 3 different metal-ceramic systems: an in vitro study. *International Journal of Prosthodontics*. 2000;13(5):80.
17. Zeltser CH, DMD and Lewinstein IS. Fit of crown wax pattern after removal from the die. *J Prosthetic Dent* 1985;53:344–6.
18. A. M. Fahmy. Comparison of Marginal Fit between Collarless Metal Ceramic and two all Ceramic Restorations. *Journal of American Science* 2012;8(6):528–34.
19. Ece Tamac, Suna Toksavul. Muhittin Toman. Clinical marginal and internal adaptation of CAD/CAM milling, laser sintering, and cast metal ceramic crowns. *J Prosthet Dent* 2014;112:909–13.
20. Zhuoli Huang, et al. Clinical Marginal and Internal Fit of Crowns Fabricated Using Different CAD/CAM Technologies. *Journal of Prosthodontics* 2014;00: 1–5.
21. Nejatidanesh F, Shakibamehr AH, Savabi O. Comparison of Marginal and Internal Adaptation of CAD/CAM and Conventional Cement Retained Implant-Supported Single Crowns. *Implant dentistry*. 2016;25(1):103–8.
22. Ki-Baek Kim, Jae-Hong Kim, Woong-Chul Kim, Ji-Hwan Kim. Three-dimensional evaluation of gaps associated with fixed dental prostheses fabricated with new technologies. *J Prosthet Dent* 2014;112:1432–6.
23. Vojdani M, Torabi K, Farjood E, Khaledi A. Comparison the marginal and internal fit of metal copings cast from wax patterns fabricated by CAD/CAM and conventional wax up techniques. *Journal of Dentistry, Shiraz University of Medical Sciences*. 2013;14(3):118–29.
24. Reich S, Wichmann M, Nkenke E, Proeschel P. Clinical fit of all-ceramic three-unit fixed partial dentures, generated with three different CAD/CAM systems. *Eur J Oral Sci* 2005;113:174–9.
25. Vigolo P, Fonzi F. An In Vitro Evaluation of Fit of Zirconium-Oxide-Based Ceramic Four-Unit Fixed Partial Dentures, Generated with Three Different CAD/CAM Systems, before and after Porcelain Firing Cycles and after Glaze Cycles. *Journal of Prosthodontics* 2008;17: 621–6.
26. Beuer F, Nemeier P, Naumann M. Marginal fit of 14-unit zirconia fixed dental prosthesis retainers. *J Oral Rehabilitation* 2009; 36: 142–9.
27. Kohorst P, Brinkmann H, Li J, Borchers L, Stiesch M. Marginal accuracy of four-unit zirconia fixed dental prostheses fabricated using different computer-aided design/computer-aided manufacturing systems. *Eur J Oral Sci* 2009; 117: 319–25.
28. Torabi Ahangari A, Farahi L. Marginal and Internal Fit of CAD/CAM and Slip-Cast Made Zirconia Copings. *J Dent Res Dent Clin Dent Prospect* 2012; 6(2):42–8.
29. Ki-Baek Kim, et al. An evaluation of marginal fit of three-unit fixed dental prostheses fabricated by direct metal laser sintering system. *Dental Materials* 2013; 29:91–6.
30. Giordano RA. Dental ceramic restorative systems. *Compendium of Continuing Education in Dentistry* 1996; 17: 779–82.
31. Gardner FM. Margins of complete crowns—literature review. *The Journal of prosthetic dentistry*. 1982;48(4):396–400.
32. Shillingburg HT, Hobo S, Fisher DW. Preparation design and margin distortion in porcelain-fused-to-metal restorations. *The Journal of prosthetic dentistry*. 1973;29(3):276–84.
33. Buchanan WT, Svare CW, Turner KA. The effect of repeated firings and strength on marginal distortion in two ceramometal systems. *The Journal of prosthetic dentistry*. 1981;45(5):502–6.
34. Bryant RA, Nicholls JL. Measurement of distortions in fixed partial dentures resulting from degassing. *The Journal of prosthetic dentistry*. 1979;42(5):515–20.

### How to cite this article:

Mohammadi D, Movahedzadeh M, Zahra S, Hoseini SA, Iraj MB. Adaptation in metal-ceramic and all-ceramic restorations. *J Clin Anal Med* 2017;8(suppl 4): 448–53.